


FOOTPRINT ON SLICER FOR 50MM DEFOCUS AT AO STIMULUS

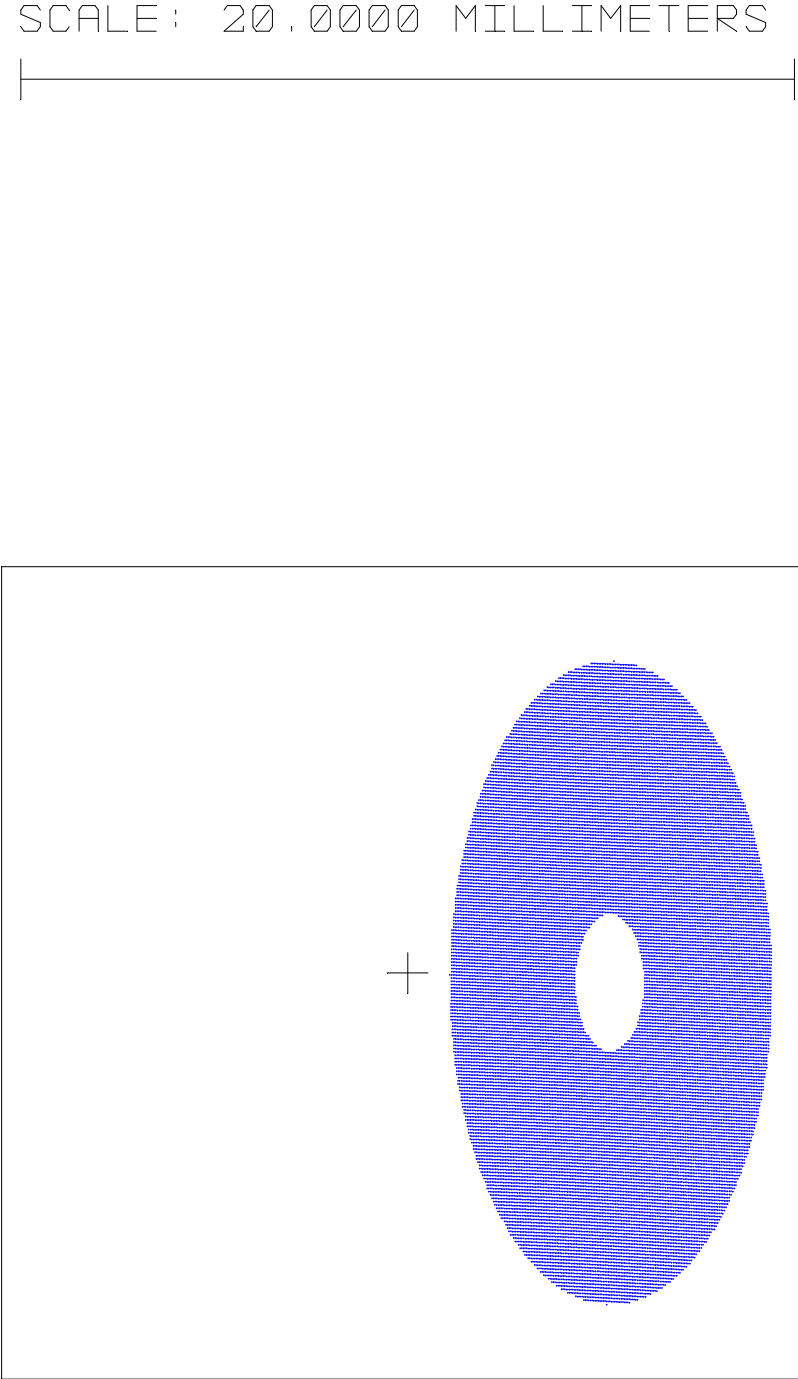

APERTURE FULL X WIDTH : 21.0000
APERTURE FULL Y HEIGHT : 21.0000
% RAYS THROUGH = 95.37%

FOOTPRINT DIAGRAM

ACQ CAMERA WITH ACCESSIBLE PUPIL	
WED AUG 2 2006	
SURFACE 63: MGSU FOCUS	
RAY X MIN =	-8.0647 RAY X MAX =
RAY Y MIN =	1.0888 RAY Y MAX =
MAX RADIUS =	10.4759 WAVELENGTH =
UNIVERSITY OF OXFORD	
DENYS WILKINSON BUILDING	
KEBLE ROAD, OXFORD, OX1 3RH	
CONFIGURATION 1 OF 1	
PALAD_CS_060306_PREOPT73.ZMX	